


OSA Specifications Explained


To understand the technical specifications of an Optical Spectrum Analyser (OSA), it is important to appreciate its basic operation. The simplest approach is to regard the OSA as an instrument that consists of two main components, i.e. a monochromator and a photodetector.

By Optical product marketing team, Yokogawa Europe

The monochromator is simply an optical bandpass filter, i.e. of all the offered input wavelengths it allows only a narrow portion to pass. The photodetector measures the power (level) of the light that passes through the monochromator.

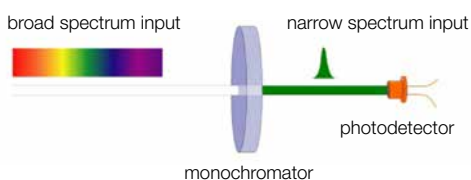

What is special about the monochromator is that it is able to (repeatedly) sweep the centre-wavelength of the bandpass filter, allowing the photodetector to record a complete optical spectrum.

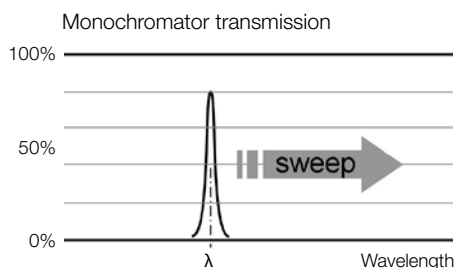


Essentially, the OSA specifications describe the performance of this measuring method. They describe for example; the accuracy, shape, speed and repeatability of the sweeping bandpass filter, but also the accuracy and linearity of the photodetector circuit.

In this article, the basis of each OSA specification is explained, together its relevance for specific applications and industries.

Span

The specification for the span of the OSA describes the minimum and maximum wavelength range that the OSA can cover with a single spectrum.

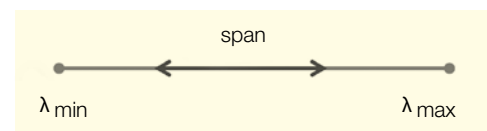

The maximum span is the complete wavelength range that the OSA can cover.

Notice that the possibility for “span = 0” is mentioned separately in the specification. In this setting, the OSA uses a fixed wavelength for the bandpass filter (i.e. no wavelength sweep). The display of the OSA now shows the measured optical power (y-axis) versus time (x-axis) rather than wavelength.

Main applications / Industries:


All

Related specifications:

All

Wavelength accuracy

This specifies the maximum wavelength error of the OSA. This specification is important for applications where the absolute wavelength value is measured.

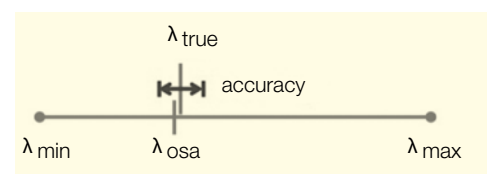

Main applications / Industries:

Analysing filters, Fibre Bragg Gratings.

Testing and adjustment of lasers


Related specifications:

Wavelength linearity

Wavelength repeatability

Wavelength linearity

The wavelength linearity of the OSA specifies the amount by which different measured wavelengths can vary from their true values. The specification provides the limits in the deviation from a straight line. Wavelength linearity is important for applications where the interval between two wavelengths is measured (relative measurement).

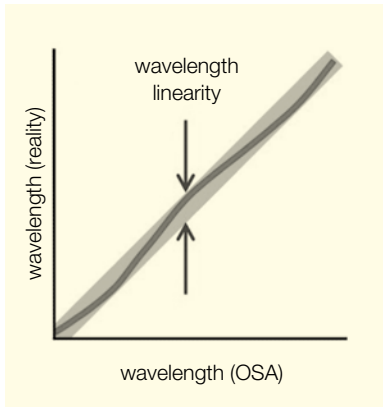


Main applications / Industries: Analysing filters, Fibre Bragg Gratings, laser output.

Related specifications: Wavelength accuracy, Wavelength repeatability

Wavelength repeatability

Specifies how accurately the OSA returns to a previously visited wavelength. This is Important for reproducing (repetitive) measurements.

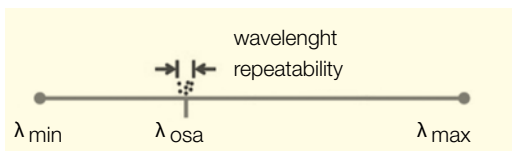

Main applications / Industries:

Manufacturing of optical parts (laser diodes, filters, fibre Bragg gratings)


Related specifications:

Wavelength linearity
Wavelength accuracy

Wavelength resolution setting

Specifies the available resolution settings on the OSA. Each resolution setting should be considered as an indication of the actual resolution used for the measurement.

Each setting corresponds to a specific exit slit size of the monochromator (see image). The actual spectral resolution used in the

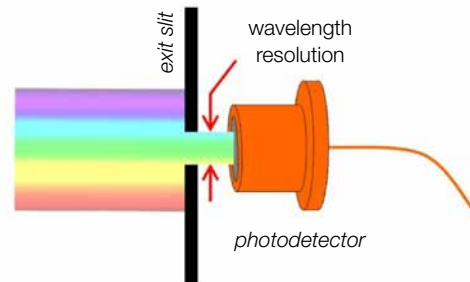

A high resolution (narrow exit slit) in combination with a narrow core input fibre is important to resolve fine spectral detail.

A low resolution (wide exit slit) is important for accurate measurements of the optical power inside a broad spectral peak (e.g. a modulated signal). The complete peak falls through the wide exit slit, meaning that one sample (small measurement error) is sufficient for measurement.

Main applications / Industries:

Telecom signal analysis, laser development (analysing laser modes)


Related specifications:

Applicable fibre

Sweep speed

The speed at which the OSA completes a wavelength sweep (typically specified for measurement over a 100nm span).

The sweep speed is especially important when performing many repetitive measurements (e.g. in manufacturing).

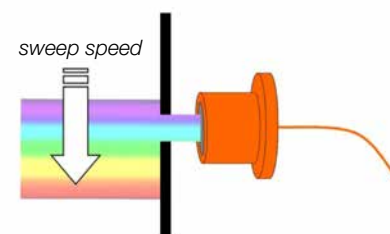

Main applications / Industries:

Manufacturing, i.e. repetitive measurements where time is money

Related specifications:

Sweep speed, Level sensitivity setting, Number of sampling


Min. sampling resolution

The smallest wavelength step size that can be selected to scan through the spectrum.

In "auto setup" (default), the OSA will select a suitable wavelength step size, based on the selected resolution setting.

In manual setup the step can be varied.

A small step size means that narrow spectral features are properly recorded. This draws a relation between sampling resolution and spectral resolution

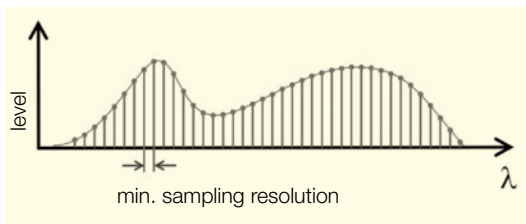

Main applications / Industries: all

Related specifications:


Span
Number of sampling

Number of samples

Specifies the minimum and maximum number of samples that the OSA can use to record a complete spectrum.

With a smaller number of samples, the OSA is able to complete the spectral sweep in less time (faster sweep speed). The trade-off is the possibility of missing fine spectral detail.

By default, the OSA automatically calculates the number of samples used for the recording, based on the span and the wavelength resolution setting of the OSA. The OSA will record 5 samples per resolution value of the OSA, so each sample has spectral overlap with multiple neighbouring samples.

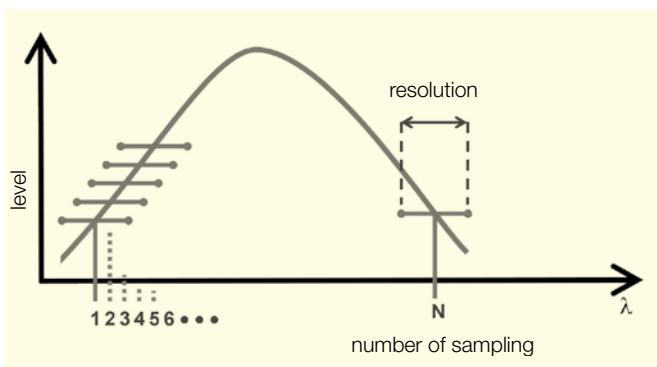

It follows that the number of samples used for the trace

$$\text{is given by } \# \text{ samples} = \frac{\text{span}}{\left(\frac{\text{resolution}}{5}\right)} + 1$$

For example; There will be 501 samples for a trace with a span of

100nm and a resolution of 1nm.

Manually the user can deviate from this by e.g. moving to a larger step size. This will reduce the number of samples and hence increase the measurement speed.

Main applications / Industries:

all

Related specifications:

Sweep speed, wavelength resolution setting, span


Level sensitivity setting

This specification describes the different circuits that are available to amplify the photodetector signal.

Each amplifier circuit has its own signal gain and response time.

A high sensitivity corresponds to a high-gain circuit with a relatively slow time response (long integration time), resulting in a relatively slow sweep speed. This setting is important for applications involving a very weak input signal.

On the other hand, a low sensitivity setting offers a fast sweep speed with a trade-off on the signal gain.

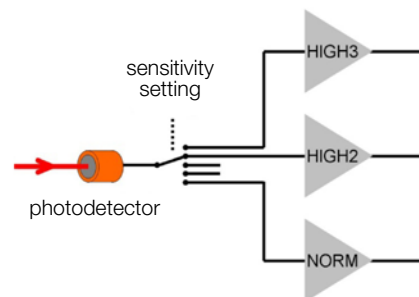

Main applications / Industries: all


Related specifications:

Sweep speed

High dynamic mode

Expresses the technique that can be used to reduce the stray light contribution from the measurement.

The parts and housing of the monochromator are coated black to keep the amount of stray light to a minimum. To reduce the influence of the remaining amount of stray light, first only the amount of stray light is measured, after which it is subtracted from the actual measurement.

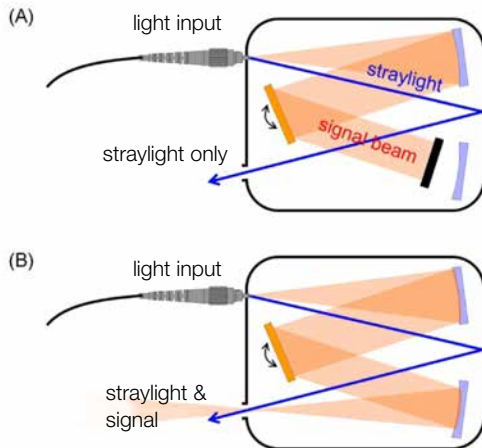

The stray light contribution is measured by blocking the signal beam, see Figure (A). This allows only stray light to exit the monochromator and reach the photodetector.

Switch Mode

When "Switch mode" is selected, the OSA will record a complete trace of stray light (A), followed by a complete "normal" measurement trace (B).

The stray light trace is subtracted from the measurement trace, and the result is displayed on screen as the end result.

Main applications / Industries:


Telecom, laser research

Related specifications:

Dynamic range

Level sensitivity

Level sensitivity expresses the minimum amount of light that can be detected by the internal photodetector. A lower light level will be lost in the detector noise.

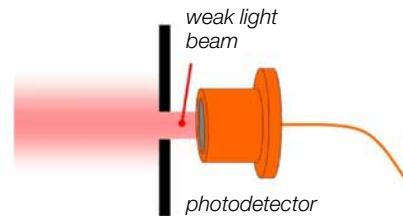


Main applications / Industries:

Filter testing, cross-talk measurement

Maximum input power

The maximum amount of light (power) that can be handled by the internal photodetector.

For narrow spectrum light like lasers, this is the all laser power within a resolution (the complete laser line falls through the monochromator exit slit). You can read it as "+20dBm per laser mode" or "+20dBm per laser line"

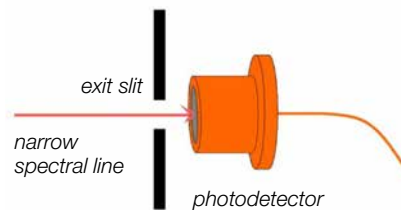

Main applications / Industries: all


Related specifications:

Maximum safe input power

Maximum safe input power

This is total maximum power that can be injected into the OSA. This can also be very broadband light.

Besides the photodetector, the depolarizer is also sensitive to high optical power. This optical component is located immediately after the entrance to the monochromator.

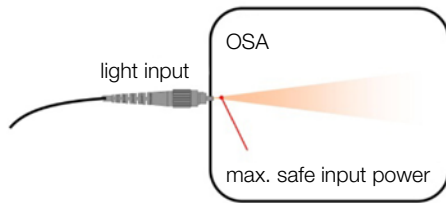

Main applications / Industries:


all

Related specifications:

Maximum input power

Level accuracy

Expresses the accuracy of the OSA for measuring optical power (level). This specification is important for applications that require measurement of the absolute amount of the optical power.

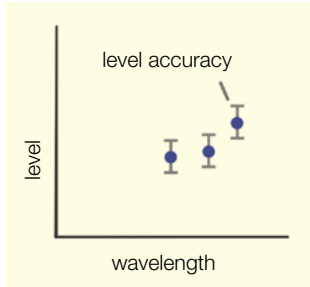

Main applications / Industries:

Telecom (signal/noise analysis)

Laser development (e.g. analysis of side modes)


Related specifications:

Level linearity, Level flatness

Level linearity

The level linearity of the OSA specifies the amount by which different measured power values vary from their true values. The specification provides the limits in the deviation from a straight line


This is Important for applications that require comparison of different level values (relative measurement)

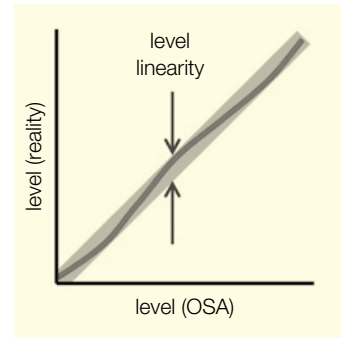

Level flatness

A perfectly flat power density spectrum should produce a perfectly horizontal (flat) OSA recording. This specification tells how well the OSA approximates this perfectly flat trace.

This is important for applications that require the comparison of level values, measured at different wavelengths.

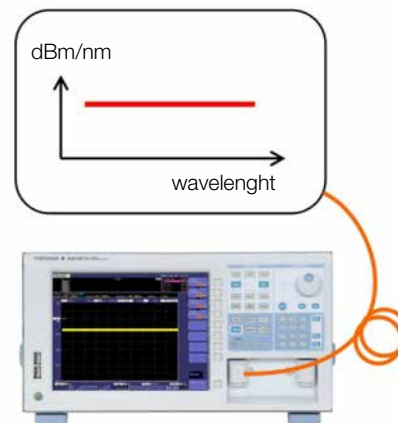

Main applications / Industries:


Telecom, optical component testing

Related specifications:

Level accuracy, Level linearity


Dynamic range

Describes the ability of the OSA to suppress the influence of neighbouring wavelengths on each sample. It is an important specification for applications that require the measurement of a weak optical signal next to a strong signal (e.g. laser line). The signal contribution from a neighbouring wavelength causes a blurring of the recorded spectrum. Therefore, the dynamic range specification is important for applications that require a very high spectral resolution.

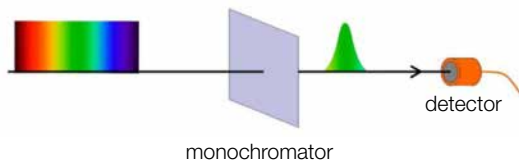

The OSA monochromator acts as a (narrow) bandpass filter (see image). It is the width and shape of the filter that is defined by the dynamic range specification (sometimes referred to as the "optical rejection ratio")

The filter shape is closely related to the resolution setting of the OSA, and the diameter of the input fibre. For the highest suppression of neighbouring wavelengths (narrowest filter) the highest resolution should be selected, and a narrow core (single mode) input fibre should be used.



Main applications / Industries:

Telecom: Signal-to-Noise measurement on DWDM signals, Noise Figure measurement (amplifier analysis)

Related specifications:

Stray light suppression
Spectral resolution setting
Applicable fibre

Stray light suppression ratio

Stray light is light that contributes to the detector signal, that is of a different wavelength than the selected wavelength. I.e. it is light that ideally should not reach the photodetector. Stray light potentially can obscure very weak optical signals in the vicinity of a strong spectral peak (e.g. laser line).

Main applications / Industries:

Telecom (OSNR, NF measurement), spectroscopy

Related specifications:

Dynamic range, High dynamic mode

Optical Return Loss (ORL)

Specifies the portion of the OSA input light that is reflected back towards the signal source (expressed in dB).

Back-reflection can cause instability of the laser source, and therefore introduce an error in the measurement.

Note: The optical return loss can be significantly improved by moving from the PC-type to an (angled) APC type fibre connector.



Main applications / Industries:

Laser research or development, telecom, i.e. all applications involving analysis of laser output

Related specifications:

Polarization dependency, Optical connector

Applicable fibre

All types of fibre (with diameters up to 800 microns) can be physically connected

The amount of light that passes through the monochromator (optical throughput) depends on the divergence angle of the input fibre (its Numerical Aperture). As the amount of light that reaches the photodetector determines the measured optical power, the type of input fibre has an effect on the optical power measured by the OSA.

The level measurement of the OSA is calibrated for a single mode (9.5/125) input fibre. When a different input fibre is used the level measurement of the OSA will have a slight offset, which is described in the user manual, and this compensation can be applied in the in the OSA level offset settings.



Main applications / Industries:


All OSA applications

Optical connector

The OSA is supplied with two (replaceable) connector adapters, one for the light input and one for the calibration light source. Three different connector adapters are available; for FC, SC or ST type fibre connectors.



The OSA connector adapters are exchangeable, and can therefore be changed as necessary. Note that the light input of the OSA accepts both PC and APC (angled) fibre connectors.

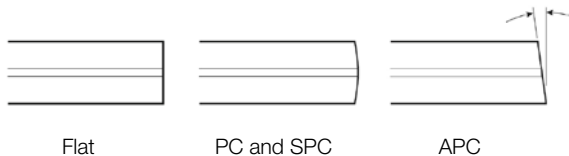

Main applications / Industries:

All OSA applications

About Yokogawa Test & Measurement

Yokogawa has been developing measurement solutions for over 100 years, consistently finding new ways to give R&D teams the tools they need to gain the best insights from their measurement strategies. The company has pioneered accurate power measurement throughout its history. In 2002 it became a leading supplier of optical Test & Measurement instruments following the acquisition of Ando Electric. Today, with more than 30 years of experience in optical testing, Yokogawa offers a broad range of optical instruments and is the market leader for Optical Spectrum Analysers in research and test laboratory environments.

Yokogawa instruments are renowned for maintaining high levels of precision and for continuing to deliver value for far longer than the typical shelf-life of such equipment. Yokogawa believes that precise and effective measurement lies at the heart of successful innovation – and has focused its own R&D on providing the tools that researchers and engineers need to address challenges great and small.

Yokogawa takes pride in its reputation for quality, both in the products it delivers – often adding new features in response to specific client requests – and the level of service and advice provided to clients, helping to devise measurement strategies for even the most challenging environments.

The guaranteed accuracy and precision of Yokogawa's instruments results from the fact that Yokogawa has its own European standards laboratory at its European headquarters in The Netherlands. This facility is the only industrial (i.e. non-government or national) organisation to offer ISO 17025 accredited power calibration, at frequencies up to 100 kHz: a requirement for higher harmonic measurements specified in quality standards such as ISO 9000.

Meet the Precision Makers at

tmi.yokogawa.com

More information about
the world's most trusted OSAs,
visit tmi.yokogawa.com

